

100 90 80 70 60 50 40 30 20 10 0

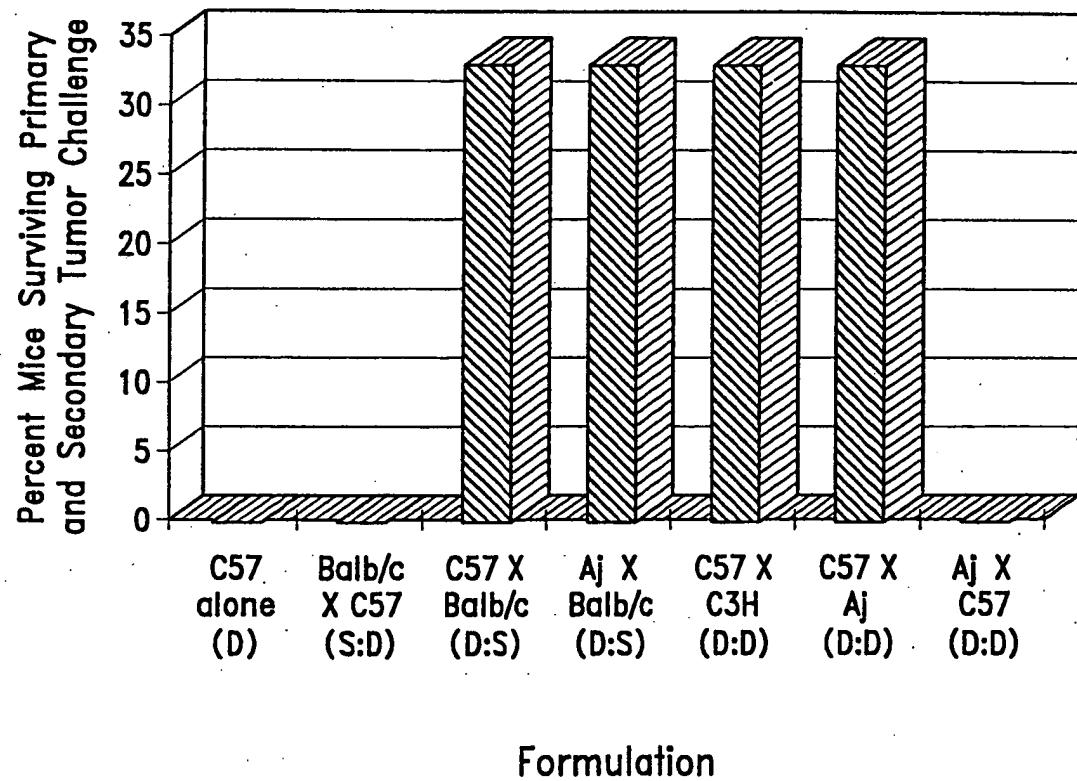


Fig. 1

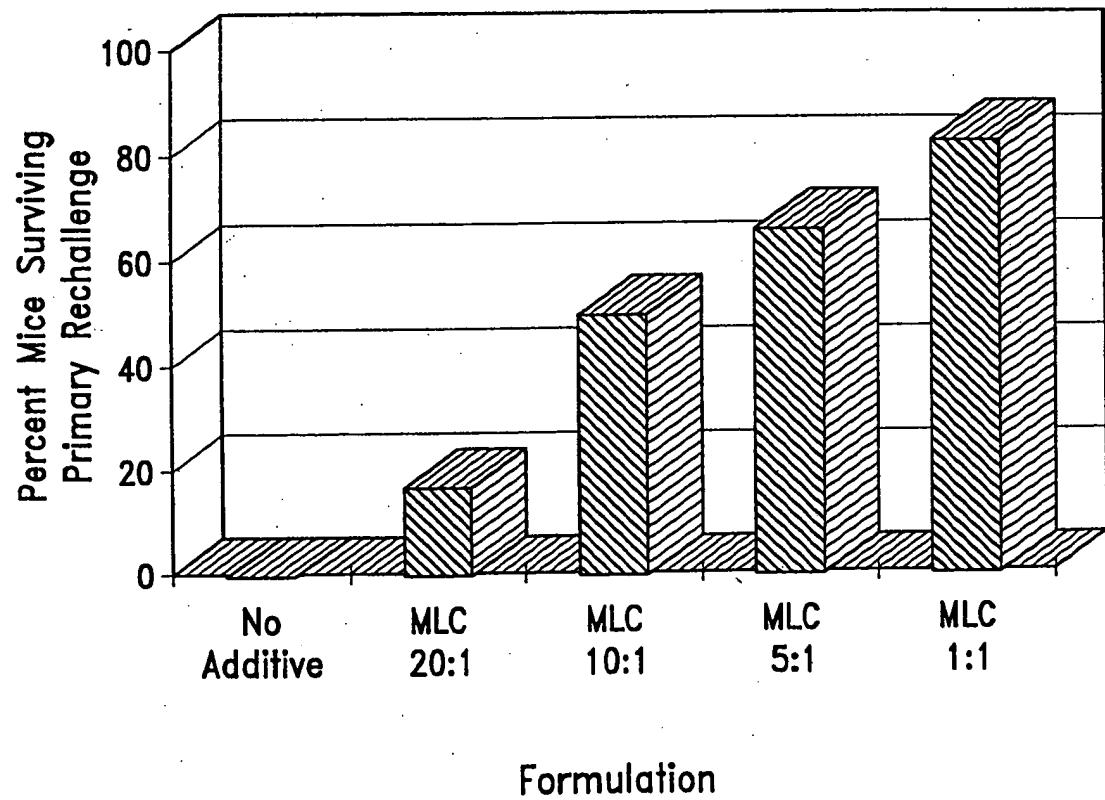


Fig. 2

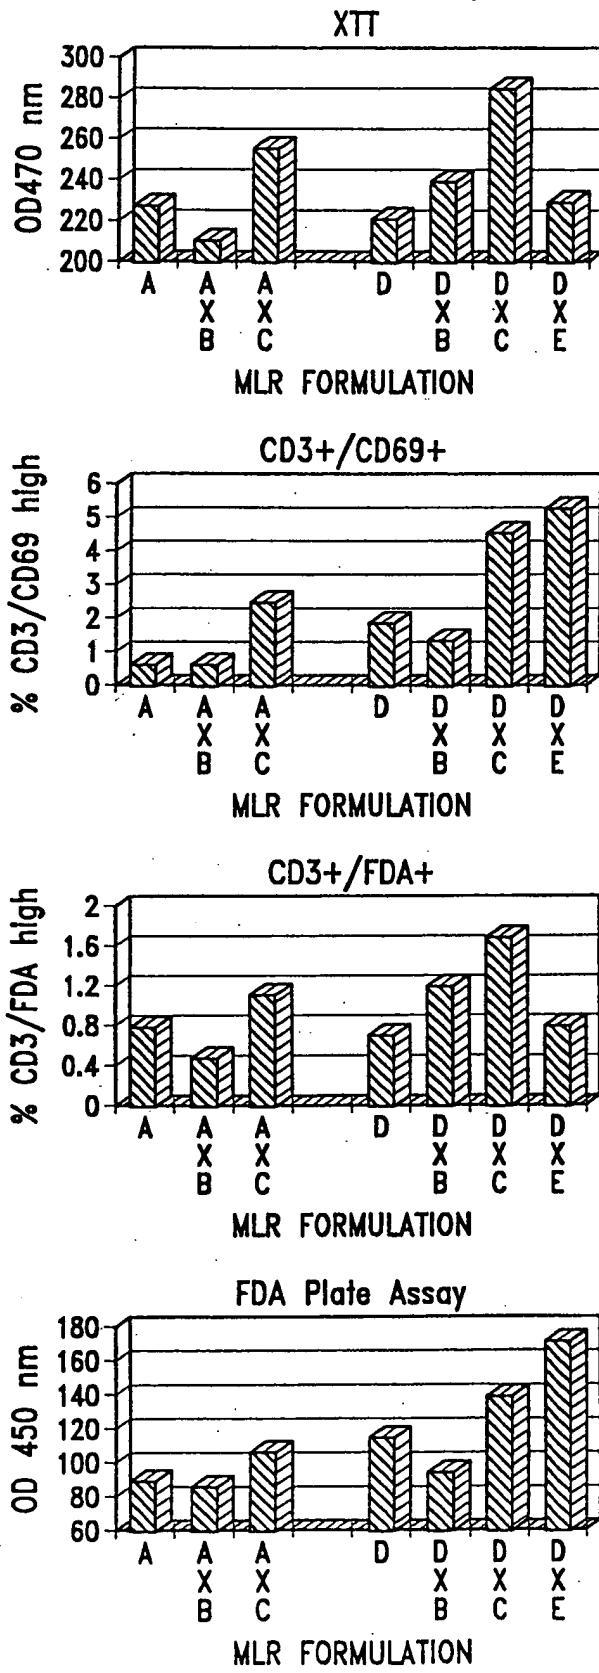


Fig. 3

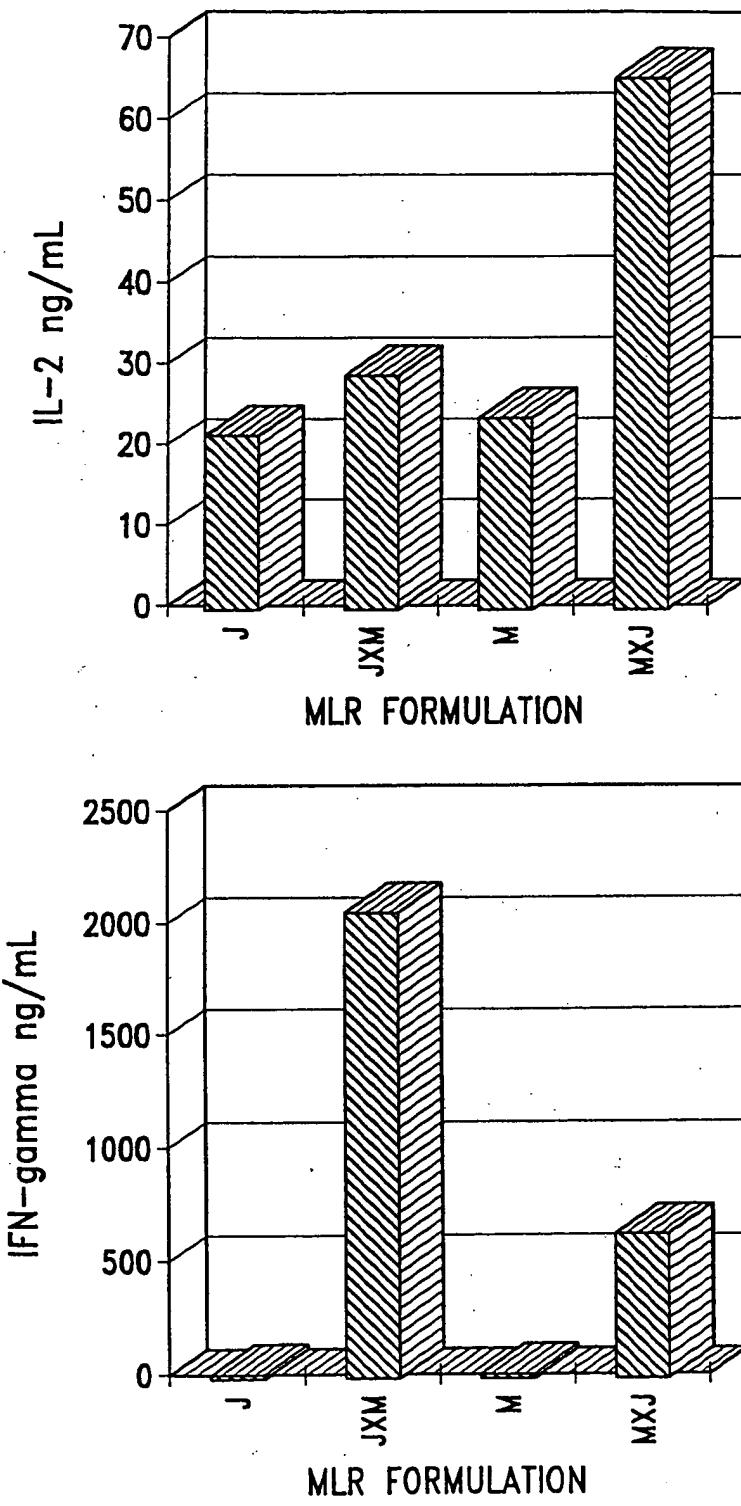


Fig. 4

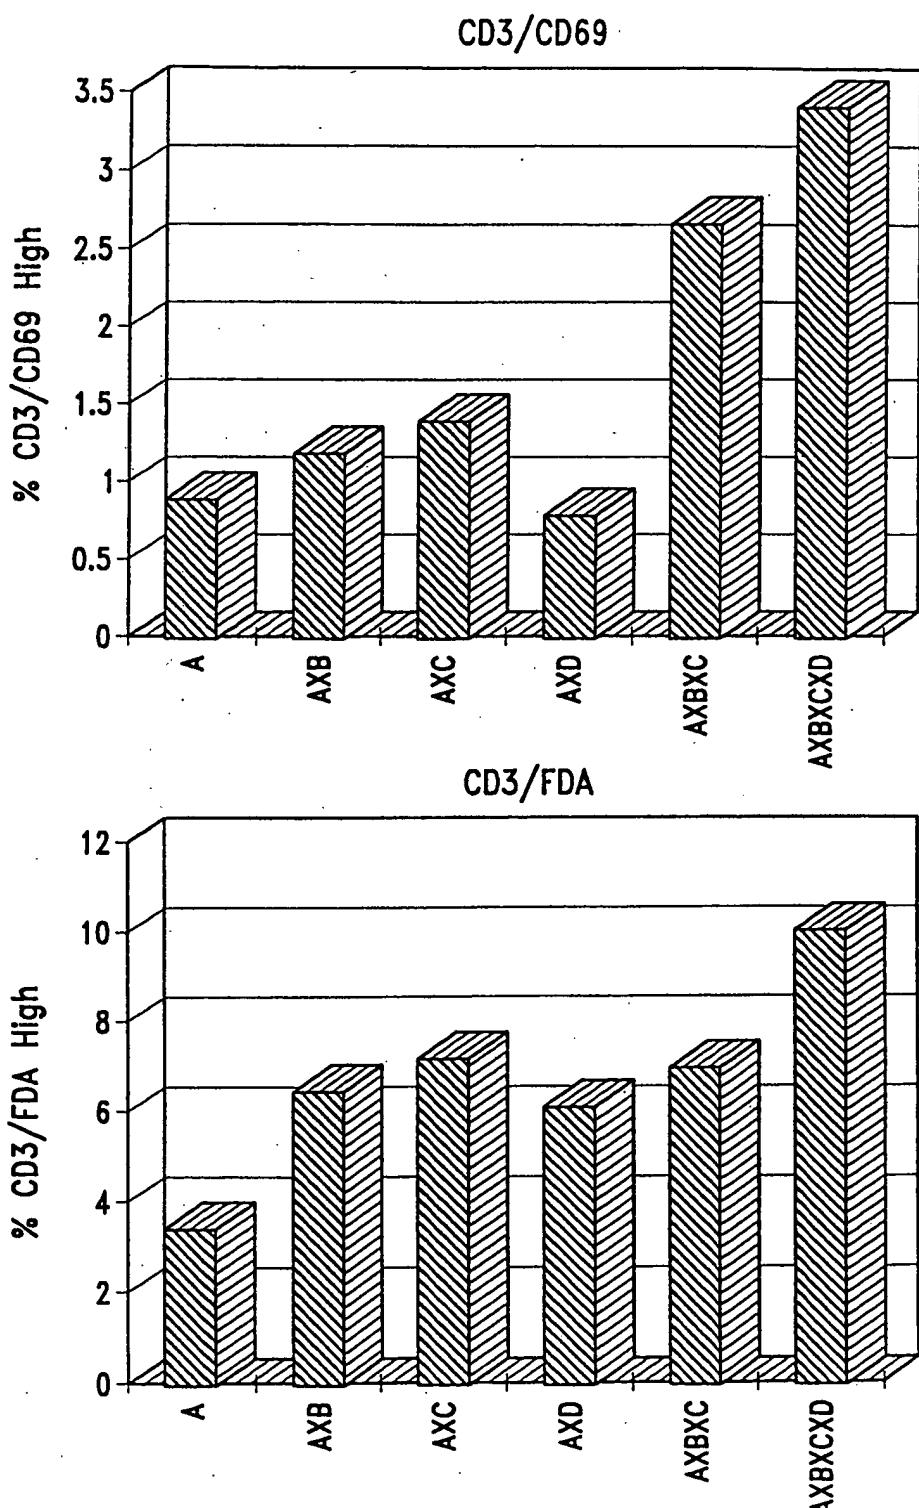


Fig. 5

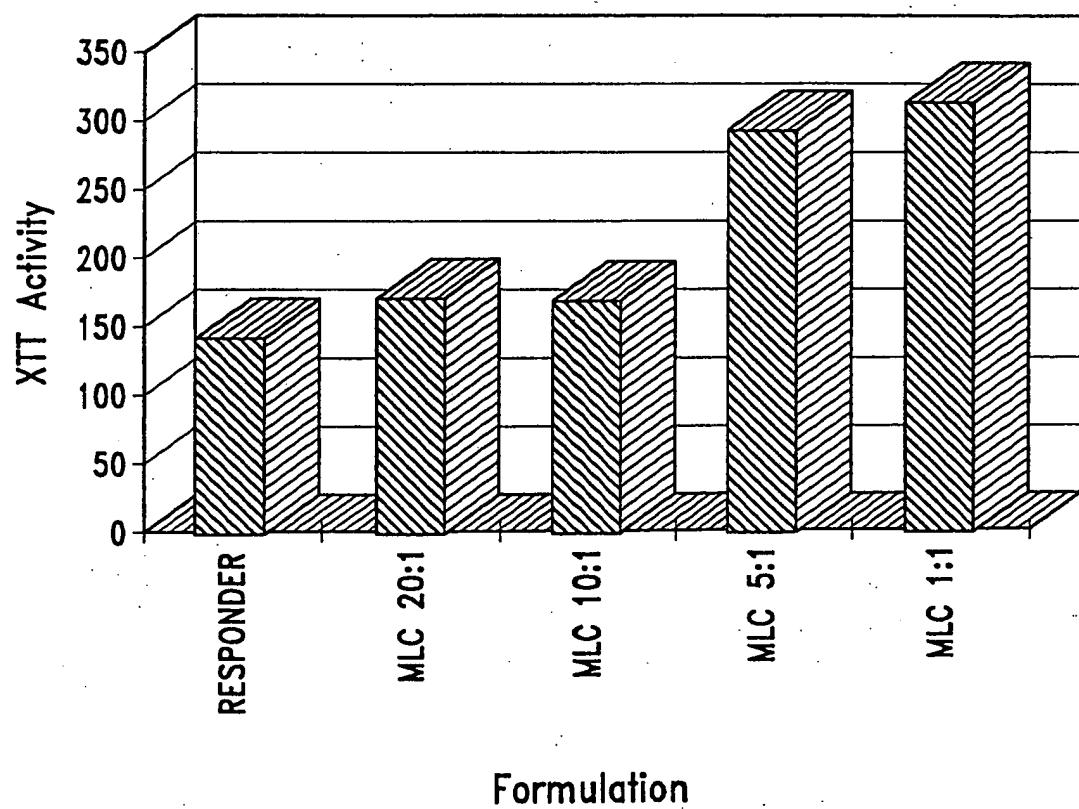


Fig. 6

DO NOT USE THIS EQUIPMENT

XTT Formazan Reduction

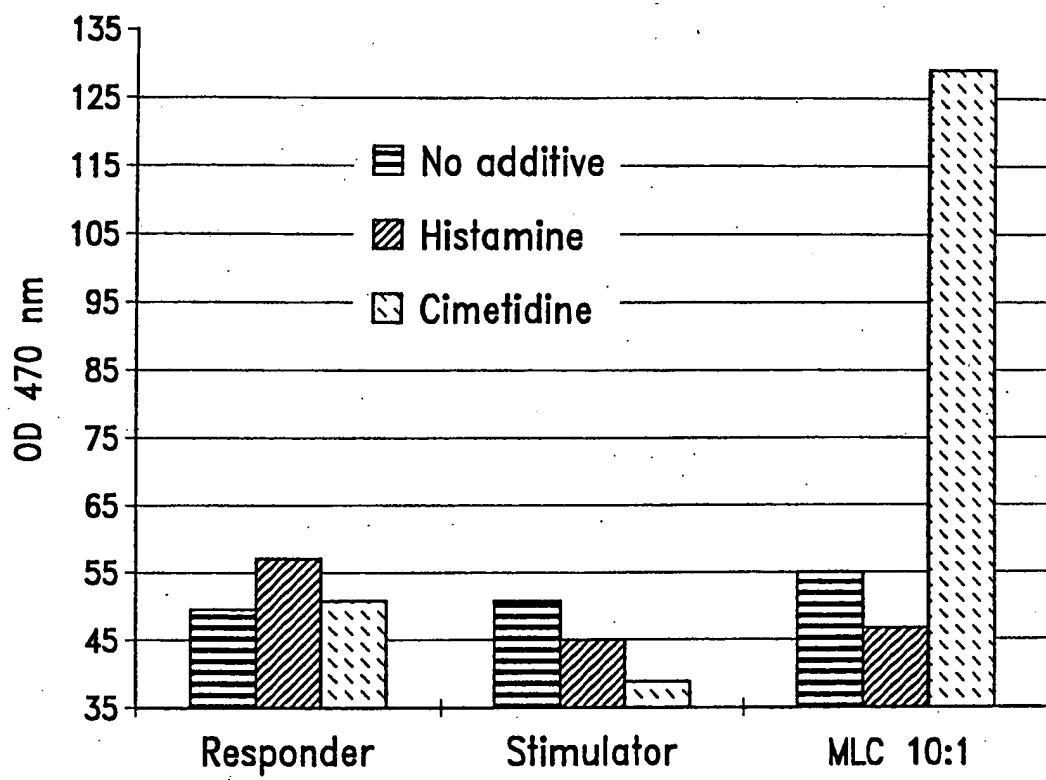


Fig. 7